

NAME ; Swapan Pradhan.

AGE/SEX :


47

Refd. by Doc. : Dr. P. M. D. H.

DATE OF REPORT : 29.06.19.

REPORT ON EXAMINATION OF BLOOD

Sample : Blood/Serum.

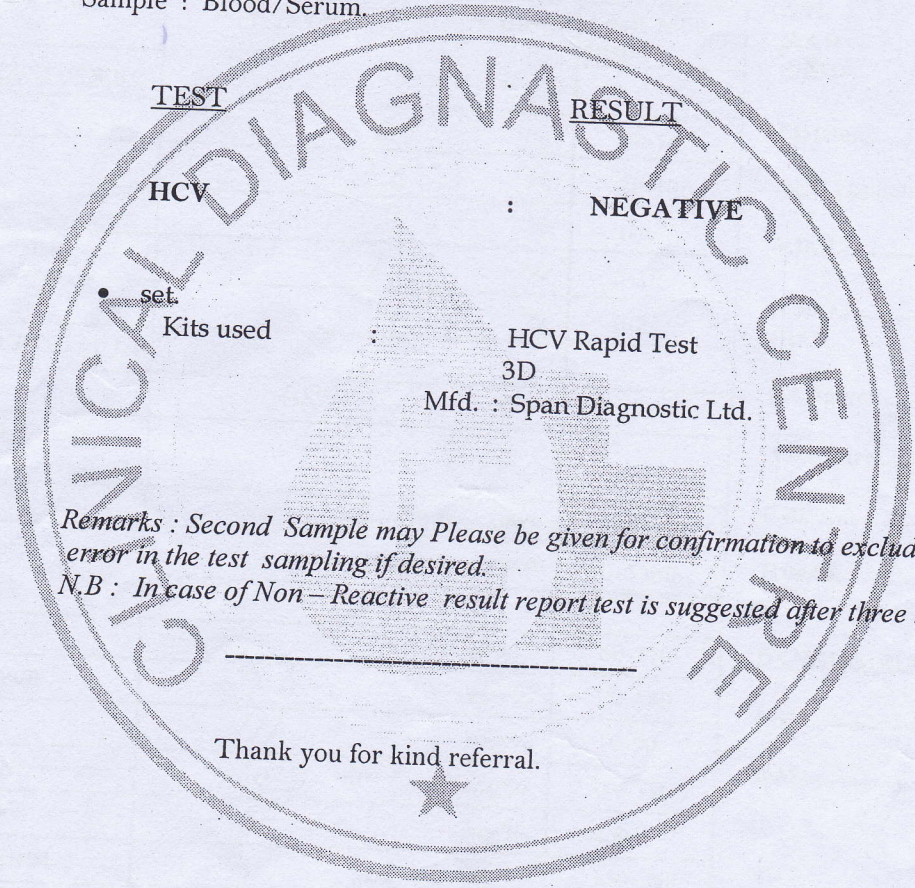

TEST

RESULT

HCV

: NEGATIVE

• set.

Kits used

: HCV Rapid Test
3D

Mfd. : Span Diagnostic Ltd.

Remarks : Second Sample may Please be given for confirmation to exclude any error in the test sampling if desired.

N.B : In case of Non - Reactive result report test is suggested after three months.

Thank you for kind referral.

Checked by :

Dr. J. Ghosh
M.D. (Path)

Dr. Anilash Das
MBBS, DCP (Cal.)

- 1) If Result is unexpected, alarming or not matched with clinical conditions please contact the lab for recheck of the Result.
- 2) The test result only to the sample collected for the test.
- 3) Identity of the patient is not varified.
- 4) Result of the test vary from lab to lab and also same. Parameters for the time to time for he same patient
- 5) Not for Medico Legal Purpose